



Joist Positions for a single Room 'H'-System

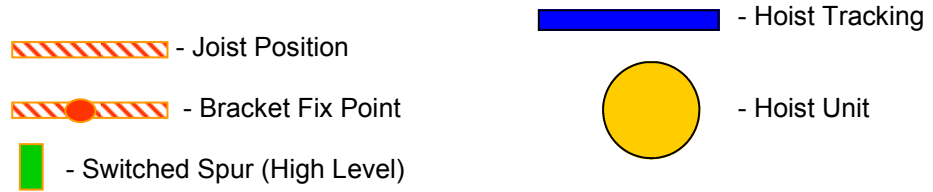


Notes

1. Joists to be a minimum of 50mm wide and capable of a point load equal to 1.5 times the Hoists SWL ie 130KG hoist requires a joist capable of supporting 195KG.
2. Lights within system to be no deeper than 20mm.

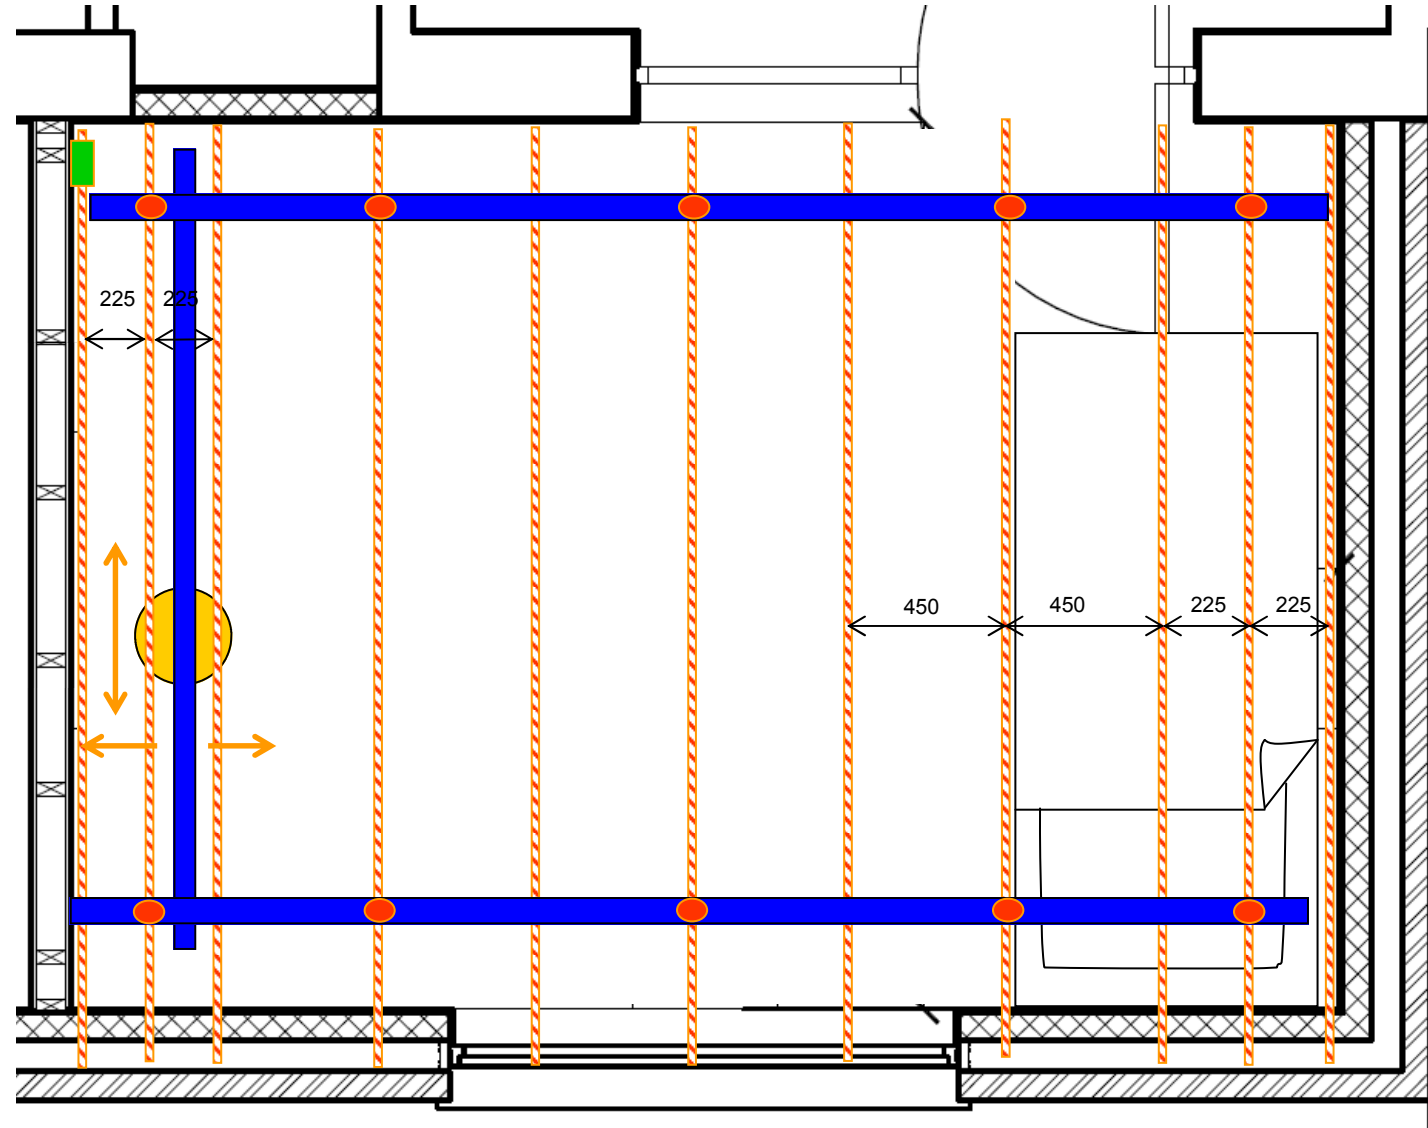


Joist Positions for a Straight track

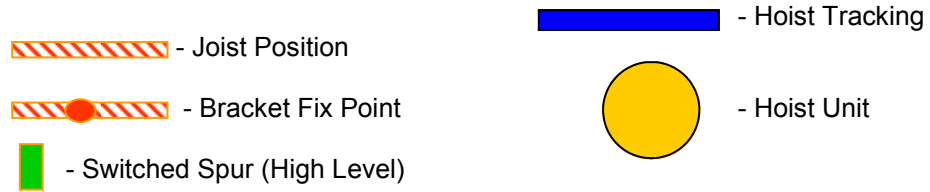


Notes

1. Joists to be a minimum of 50mm wide and capable of a point load equal to 1.5 times the Hoists SWL ie 130KG hoist requires a joist capable of supporting 195KG.
2. Lights to be at least 300mm clear of the track line.

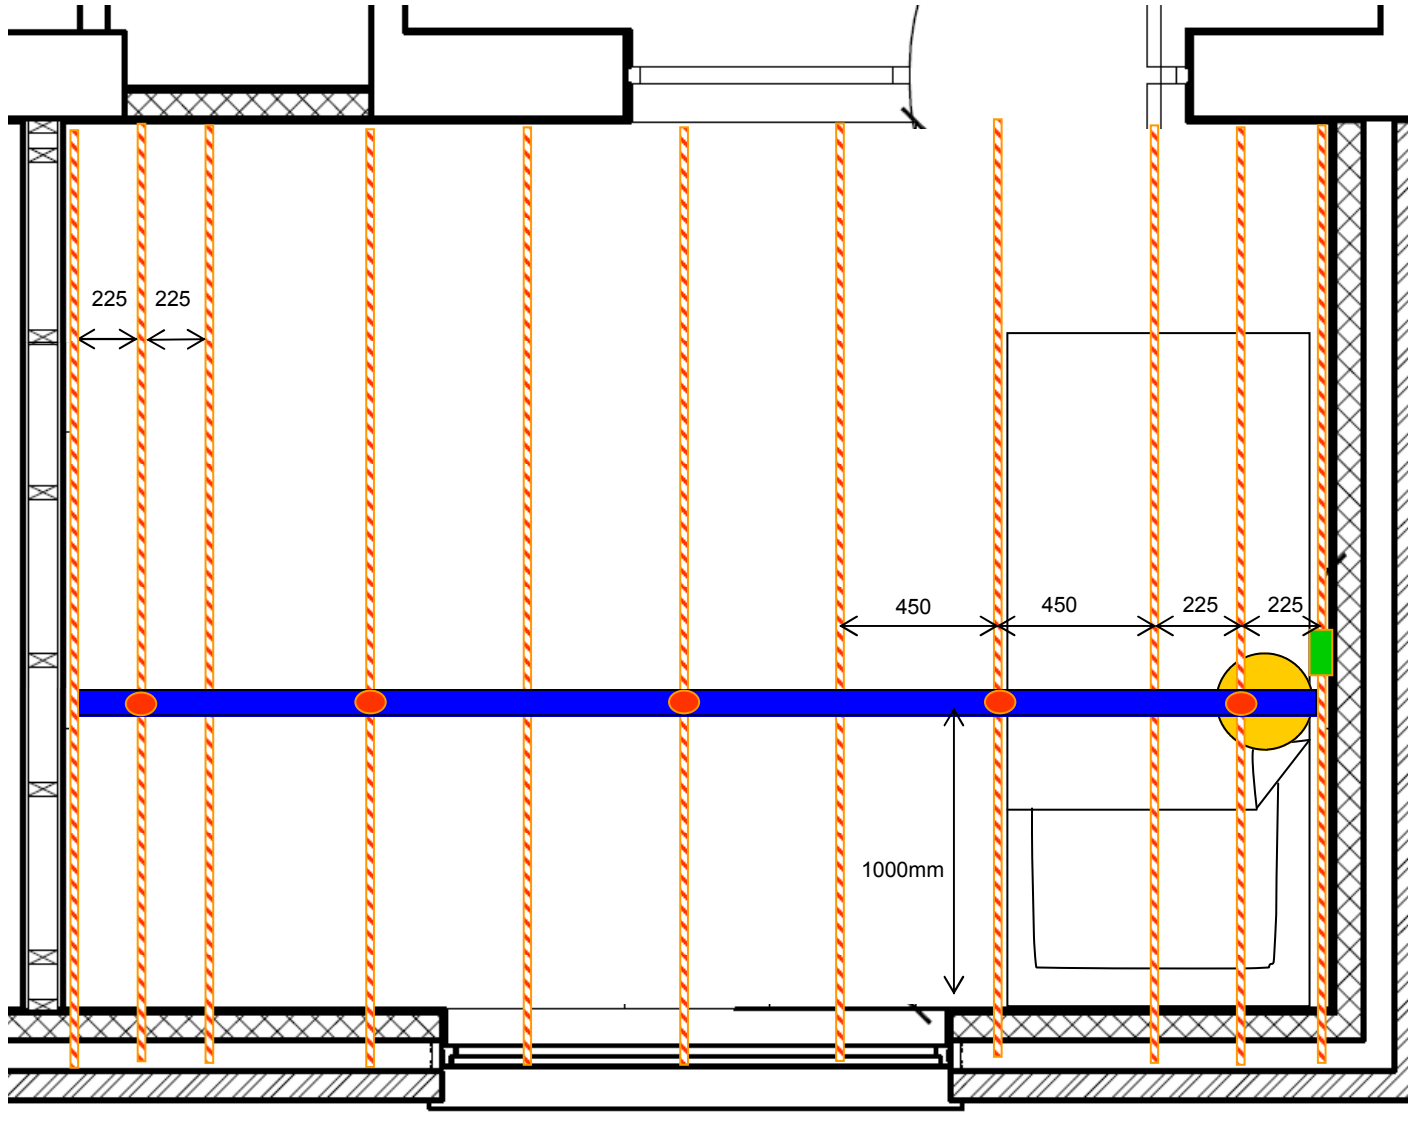

Joist Positions for a Straight track - room to room

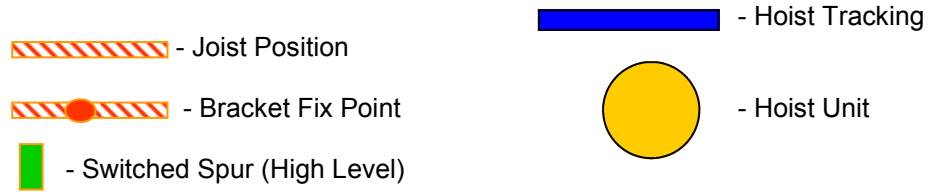

Notes

1. Joists to be a minimum of 50mm wide and capable of a point load equal to 1.5 times the Hoists SWL ie 130KG hoist requires a joist capable of supporting 195KG.
2. Lights to be at least 300mm clear of the track line.

